

## pH Measurement

pH measurement is used in a wide variety of applications: agriculture, wastewater treatment, industrial processes, environmental monitoring, and in research and development. pH is a measure of the acidity or alkalinity of a solution. The pH value states the relative quantity of hydrogen ions ( $H^+$ ) contained in a solution. The greater the concentration of  $H^+$ , the more acidic the solution, and the lower the pH. In this relationship, pH is defined as the negative logarithm of hydrogen activity.

A standard pH measuring system consists of three elements:

**pH electrode**  
**temperature compensation element**  
**pH meter or controller**

### Definition of pH

The pH value of a solution is the negative log of its hydrogen ion activity ( $\alpha$ ), which is the product of hydrogen ion concentration  $[H^+]$  and the activity coefficient of hydrogen ( $\gamma_{H^+}$ ) at that concentration.

$$pH = -\log \alpha = -\log \gamma_{H^+}[H^+]$$


In pure water and in dilute solutions, the  $H^+$  activity can be considered the same as the  $H^+$  concentration.

$$pH = -\log H^+[H^+] = -\log [H^+]$$

The pH of a solution measures the degree of acidity or alkalinity relative to the ionization of water. Pure water dissociates to yield  $10^{-7}$  M of  $[H^+]$  and  $[OH^-]$  at  $25^\circ C$ ; thus, the pH of water is 7 minus the point of neutrality.

$$pH_{\text{water}} = -\log [H^+] = -\log 10^{-7} = 7$$

Most pH readings range from 0 to 14. Solutions with a higher  $[H^+]$  than water (pH less than 7) are acidic; solutions with a lower  $[H^+]$  than water (pH greater than 7) are basic or alkaline.

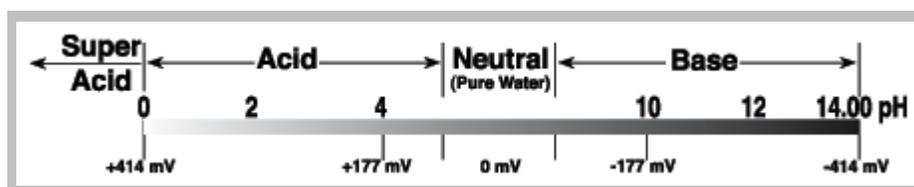

## pH Measurement

Measuring pH involves comparing the potential of solutions with unknown  $[H^+]$  to a known reference potential. pH meters convert the voltage ratio between a reference half-cell and a sensing half-cell to pH values. Today, most electrodes are combination electrodes with both the reference and sensing half-cells in the same body.

**Reference Half-Cells** contain a conductor (usually silver with a silver chloride coating) immersed in a solution with known  $[H^+]$ . The potential between this internal conductor and the known solution is constant, providing a stable reference potential.

**Sensing Half-Cells** (measuring half-cells) are made of a non-conducting glass (or epoxy) tube sealed to a conductive glass membrane. Like the reference half-cell, the sensing half-cell also contains a conductor immersed in a buffered electrolyte solution, ensuring constant voltages on the inner surface of the glass membrane and the sensing conductor.

When the pH electrode is immersed in the solution to be measured, a potential is established on the surface of the sensing glass membrane. If the unknown solution is neutral, the sum of fixed voltages on the inner surface of the glass membrane and on the sensing conductor approximately balances the voltage on the outer surface of the glass membrane and the reference half-cell. This results in a total potential difference of 0 mV and a pH value of 7.

In acidic or alkaline solutions, the voltage on the outer membrane surface changes proportionally to changes in  $[H^+]$ . The pH meter detects the change in potential and determines  $[H^+]$  of the unknown by the Nernst equation:

$$E = E^\circ + \frac{2.3RT}{nF} \log \frac{\text{unknown } [H^+]}{\text{internal } [H^+]}$$

where:

$E$  is the total potential difference (measured in mV)

$E^\circ$  is the reference potential

$R$  is the gas constant

$T$  is the temperature in Kelvin

$n$  is the number of electrons

$F$  is Faraday's constant

$[H^+]$  is hydrogen ion concentration

***Fann Instrument Company offers a complete line of pH Meters, pH Electrodes, supplies and accessories for use in testing drilling fluids in accordance with the following***

***American Petroleum Institute publications:***

**API Recommended Practice 13B-1, ANSI/API 13B-1/ISO 10414-1,**

**API Recommended Practice 13B-2, & API Specification 13A**

Visit our Website: [www.fann.com](http://www.fann.com)